


HbA1c: Nessun dato

Microinf: Paradigm Veo - 554
Sensore: In uso

#758314

Dati sensore (mg/dl)

04/03/10 ■ 05/03/10 ■ 06/03/10 ■ 07/03/10 ■ 08/03/10 ■ Media - - -

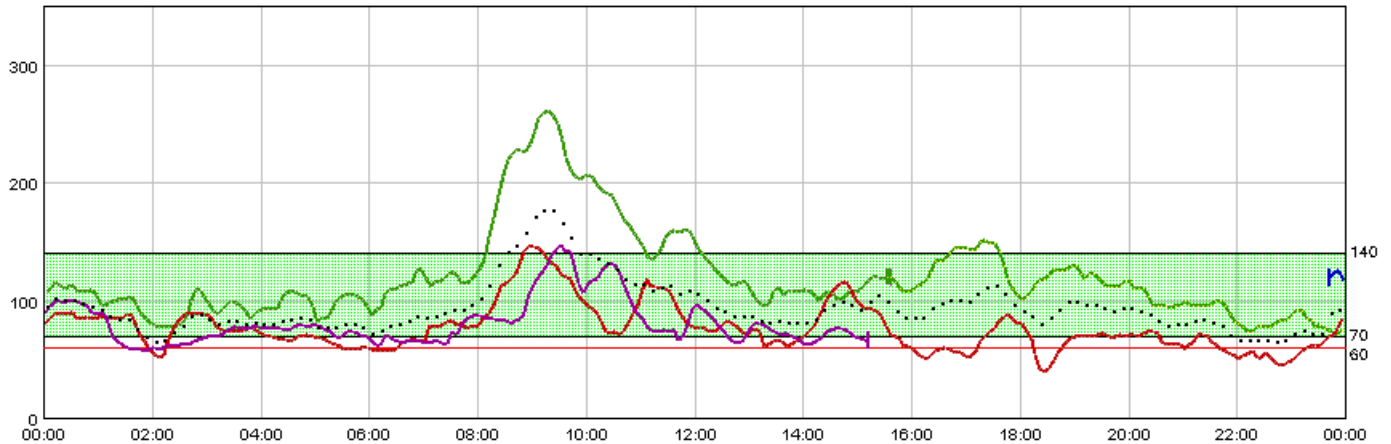

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	Media/Totale
N° di valori sensore	4	288	288	183	0	763
Glic. sensore alta (mg/dl)	125	261	146	147	N/A	261
Glic. sensore bassa (mg/dl)	117	71	40	57	N/A	40
Glic. sensore media (mg/dl)	121	120	76	81	N/A	94
Dev. standard	N/A	39	20	20	N/A	35
% MAD	N/A	9,7	18,1	25,0	N/A	15,8
N° di calibrazioni valide	1	3	4	1	0	9

Riepilogo escursioni

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	Media/Totale
N° escursioni	0	2	7	2	0	11
N° escursioni GS alta	0	2	1	1	0	4
N° escursioni ipoglicemiche	0	0	6	1	0	7
AUC sopra limite	0,0	8,7	0,1	0,1	N/A	3,3
AUC sotto limite	0,0	0,0	4,2	1,8	N/A	2,0

Durata distribuzione (hh:mm)



	04/03/10	05/03/10	06/03/10	07/03/10	08/03/10	Media/Totale
Sopra 140	0:00 0%	4:35 19%	0:20 1%	0:20 2%	N/A	5:15 8%
Entro (70 - 140)	0:20 100%	19:25 81%	14:05 59%	10:00 66%	N/A	43:50 69%
Sotto 70	0:00 0%	0:00 0%	9:35 40%	4:55 32%	N/A	14:30 23%