


HbA1c: Nessun dato

Microinf: Paradigm Veo - 554
Sensore: In uso

#757660

Dati sensore (mg/dl)

04/03/10 — 05/03/10 — 06/03/10 — 07/03/10 — 08/03/10 — Media - - -

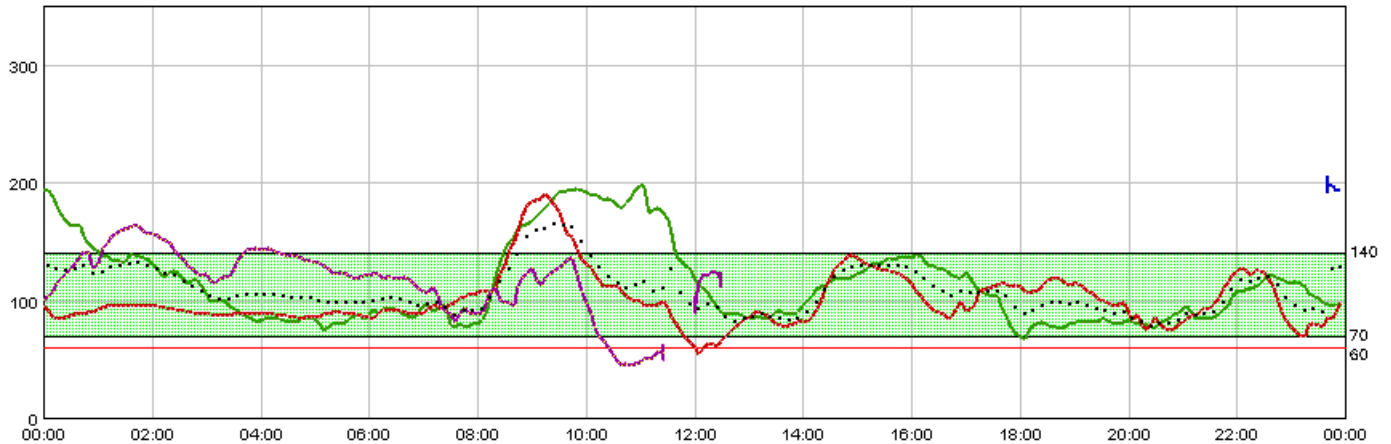

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	Media/Totale
N° di valori sensore	4	288	288	145	0	725
Glic. sensore alta (mg/dl)	198	198	190	163	N/A	198
Glic. sensore bassa (mg/dl)	193	67	55	45	N/A	45
Glic. sensore media (mg/dl)	196	114	100	116	N/A	109
Dev. standard	N/A	35	23	28	N/A	31
% MAD	N/A	13,1	15,8	N/A	N/A	14,2
N° di calibrazioni valide	1	7	5	1	0	14

Riepilogo escursioni

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	Media/Totale
N° escursioni	0	1	2	3	0	6
N° escursioni GS alta	0	1	1	2	0	4
N° escursioni ipoglicemiche	0	0	1	1	0	2
AUC sopra limite	55,5	6,5	1,6	1,9	N/A	3,9
AUC sotto limite	0,0	0,0	0,3	1,8	N/A	0,5

Durata distribuzione (hh:mm)



	04/03/10	05/03/10	06/03/10	07/03/10	08/03/10	Media/Totale
Sopra 140	0:20 100%	4:15 18%	1:20 6%	2:05 17%	N/A	8:00 13%
Entro (70 - 140)	0:00 0%	19:35 81%	21:45 90%	8:50 73%	N/A	50:10 83%
Sotto 70	0:00 0%	0:10 1%	0:55 4%	1:10 10%	N/A	2:15 4%