


HbA1c: Nessun dato

Microinf: Paradigm Veo - 554  
Sensore: In uso

#752125

### Dati sensore (mg/dl)

04/03/10 05/03/10 06/03/10 07/03/10 08/03/10 Media

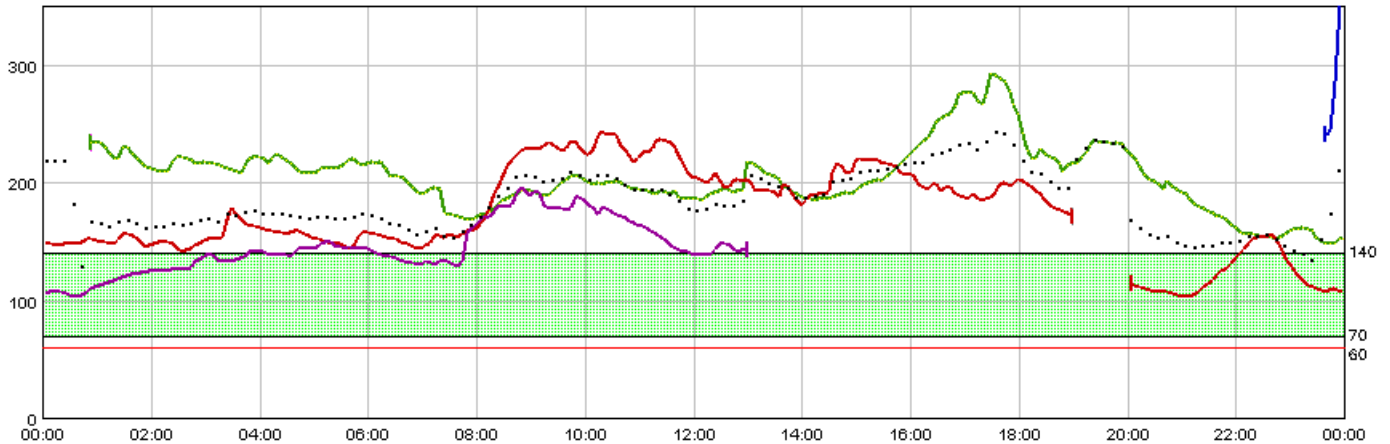

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	Media/Totale
N° di valori sensore	5	285	276	156	0	722
Glic. sensore alta (mg/dl)	396	400	244	196	N/A	400
Glic. sensore bassa (mg/dl)	241	149	103	104	N/A	103
Glic. sensore media (mg/dl)	301	210	173	145	N/A	182
Dev. standard	61	41	37	23	N/A	45
% MAD	N/A	14,2	5,7	17,5	N/A	13,2
N° di calibrazioni valide	1	4	2	1	0	8

### Riepilogo escursioni

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	Media/Totale
N° escursioni	0	1	1	3	0	5
N° escursioni GS alta	0	1	1	3	0	5
N° escursioni ipoglicemiche	0	0	0	0	0	0
AUC sopra limite	161,0	69,5	36,9	11,1	N/A	45,1
AUC sotto limite	0,0	0,0	0,0	0,0	N/A	0,0

### Durata distribuzione (hh:mm)



	04/03/10	05/03/10	06/03/10	07/03/10	08/03/10	Media/Totale
<b>Sopra 140</b>	0:25 100%	23:45 100%	19:45 86%	6:40 51%	N/A	50:35 84%
<b>Entro (70 - 140)</b>	0:00 0%	0:00 0%	3:15 14%	6:20 49%	N/A	9:35 16%
<b>Sotto 70</b>	0:00 0%	0:00 0%	0:00 0%	0:00 0%	N/A	0:00 0%