


HbA1c: Nessun dato

Microinf: Paradigm Veo - 554
Sensore: In uso

#743484

Dati sensore (mg/dl)

04/03/10 05/03/10 06/03/10 07/03/10 08/03/10 Media

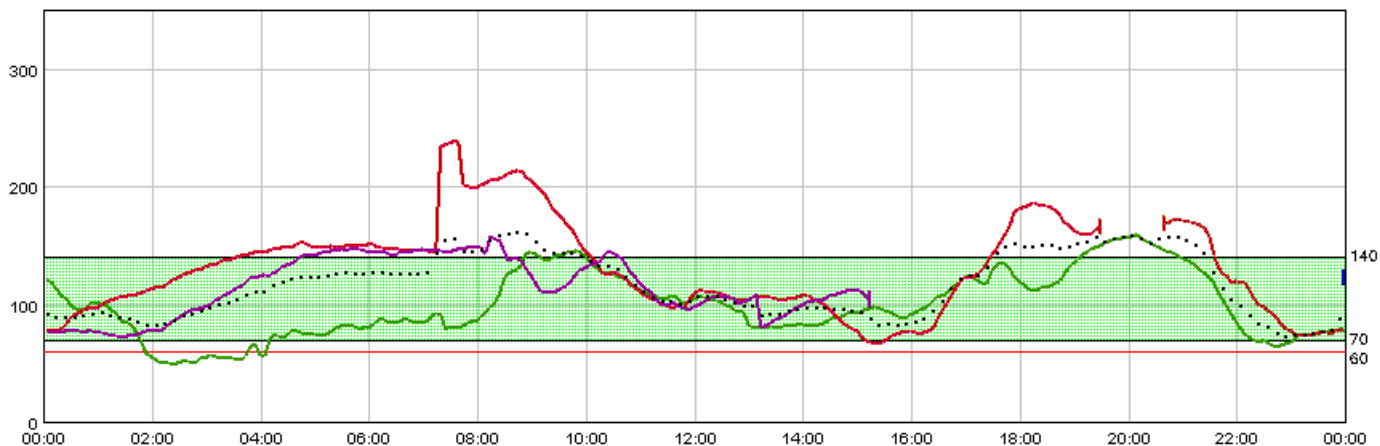

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	Media/Totale
N° di valori sensore	1	288	275	183	0	747
Glic. sensore alta (mg/dl)	123	159	239	158	N/A	239
Glic. sensore bassa (mg/dl)	123	49	67	72	N/A	49
Glic. sensore media (mg/dl)	123	99	130	115	N/A	114
Dev. standard	N/A	28	40	25	N/A	35
% MAD	N/A	13,3	47,2	31,1	N/A	28,1
N° di calibrazioni valide	0	4	3	2	0	9

Riepilogo escursioni

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	Media/Totale
N° escursioni	0	3	2	2	0	7
N° escursioni GS alta	0	2	2	2	0	6
N° escursioni ipoglicemiche	0	1	0	0	0	1
AUC sopra limite	0,0	0,9	12,2	1,5	N/A	5,2
AUC sotto limite	0,0	1,6	0,0	0,0	N/A	0,6

Durata distribuzione (hh:mm)



	04/03/10	05/03/10	06/03/10	07/03/10	08/03/10	Media/Totale
Sopra 140	0:00 0%	2:40 11%	9:35 42%	4:00 26%	N/A	16:15 26%
Entro (70 - 140)	0:05 100%	18:15 76%	13:00 57%	11:15 74%	N/A	42:35 69%
Sotto 70	0:00 0%	3:05 13%	0:20 1%	0:00 0%	N/A	3:25 5%