


HbA1c: Nessun dato

Microinf: Paradigm Veo - 554  
Sensore: In uso

#749953

### Dati sensore (mg/dl)

04/03/10 05/03/10 06/03/10 07/03/10 08/03/10 09/03/10 10/03/10 Media - - -

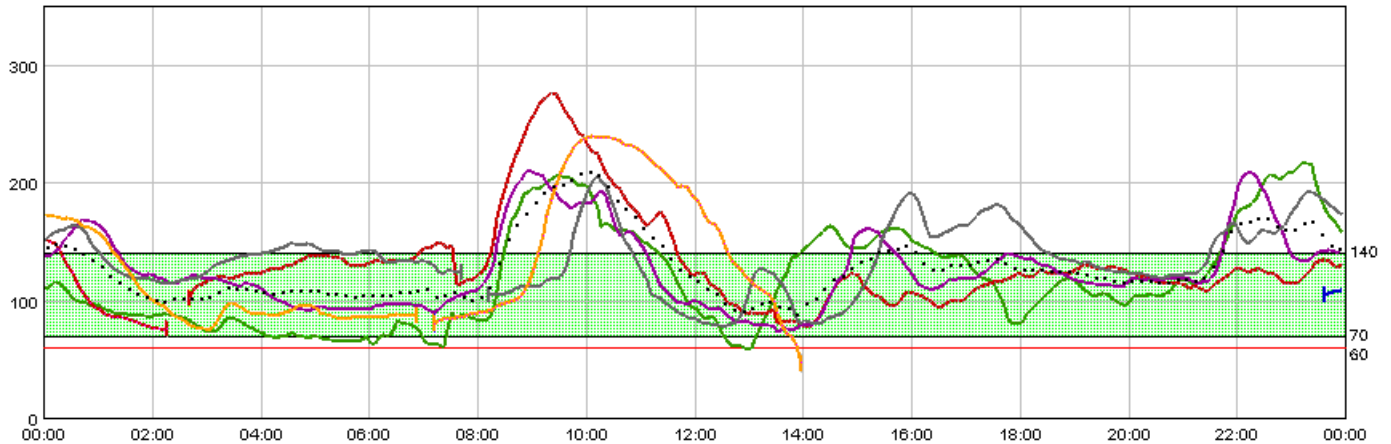

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	mar 9 mar	mer 10 mar	Media/Totale
N° di valori sensore	5	288	284	288	283	165	0	1.313
Glic. sensore alta (mg/dl)	109	217	276	211	206	240	N/A	276
Glic. sensore bassa (mg/dl)	105	58	75	74	78	47	N/A	47
Glic. sensore media (mg/dl)	107	118	130	126	135	129	N/A	128
Dev. standard	1	43	41	33	29	53	N/A	40
% MAD	N/A	16,0	25,4	7,4	4,4	N/A	N/A	15,9
N° di calibrazioni valide	1	3	4	2	2	1	0	13

### Riepilogo escursioni

	gio 4 mar	ven 5 mar	sab 6 mar	dom 7 mar	lun 8 mar	mar 9 mar	mer 10 mar	Media/Totale
N° escursioni	0	4	2	5	4	2	0	17
N° escursioni GS alta	0	3	2	5	4	1	0	15
N° escursioni ipoglicemiche	0	1	0	0	0	1	0	2
AUC sopra limite	0,0	10,4	10,9	8,4	9,3	19,3	N/A	10,9
AUC sotto limite	0,0	0,5	0,0	0,0	0,0	0,2	N/A	0,1

### Durata distribuzione (hh:mm)



	04/03/10	05/03/10	06/03/10	07/03/10	08/03/10	09/03/10	10/03/10	Media/Totale
<b>Sopra 140</b>	0:00 0%	7:35 32%	4:25 19%	6:25 27%	9:25 40%	4:50 35%	N/A	32:40 30%
<b>Entro (70 - 140)</b>	0:25 100%	13:45 57%	19:15 81%	17:35 73%	14:10 60%	8:40 63%	N/A	73:50 67%
<b>Sotto 70</b>	0:00 0%	2:40 11%	0:00 0%	0:00 0%	0:00 0%	0:15 2%	N/A	2:55 3%